



# Fetal Direct ECG monitoring made easy

## Fetal Direct ECG solution

### A fetal monitoring solution designed around you

Now there's an innovative way to improve the quality of care you deliver to mothers and their babies during labor. The new Philips fetal spiral electrodes are simple to use. Plus, our uniquely designed DECG reusable legplate adapter cable makes cleaning easier than ever.


Every part of the system—the fetal spiral electrode, reusable legplate adapter cable, and disposable attachment electrode—has been designed around the way you work.

### Safer and easier to use

Our new fetal monitoring solution meets the highest standard of safety.

A new handle features a protection tab that keeps the spiral tip inside the tube during insertion. As a result, it's unlikely that you will accidentally puncture the mother's birth canal, the fetus, or your finger tips. The protection tab also serves as a visual reference point to indicate how far the spiral has turned when attaching the electrode.

In addition, a simple connector plugs securely into the legplate adapter cable to deliver accurate, reliable heart rate readings.

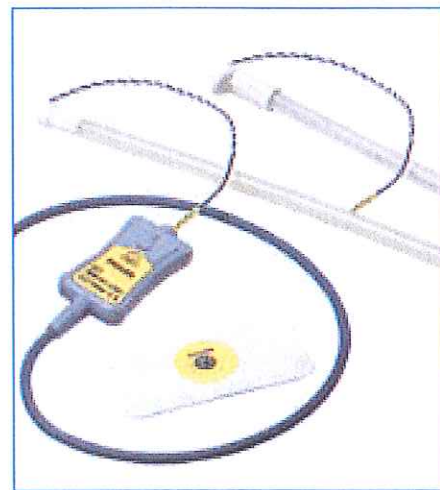

#### Single spiral electrode

Handle  
Protection tab



#### Double spiral electrode

Handle  
Protection tab



# PHILIPS



### Easy to clean

A new and improved legplate adapter cable is a one-piece, seamless design. The electronics are completely sealed, so you can safely immerse it in cleaning and disinfection fluids. The attachment electrode connection socket is also sealed, so body fluids are less likely to enter during monitoring. Finally, a convenient flushing port makes it easy to clean the inside of the connector if needed. The new Philips system is truly a great solution.

### A versatile performer


Philips new fetal monitoring system has been tested and validated to deliver accurate signals and optimal performance with all Philips and legacy Hewlett-Packard and Agilent Technologies fetal monitors. Plus, we offer legplate adapter cables to fit the most popular fetal monitors made by GE Corometrics and Spacelabs.

It's all part of Philips' commitment to bringing you the most advanced technology built to the highest standards of quality.

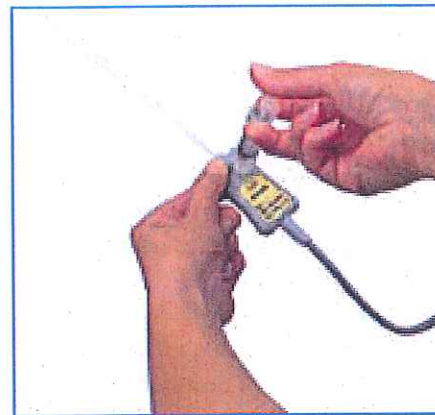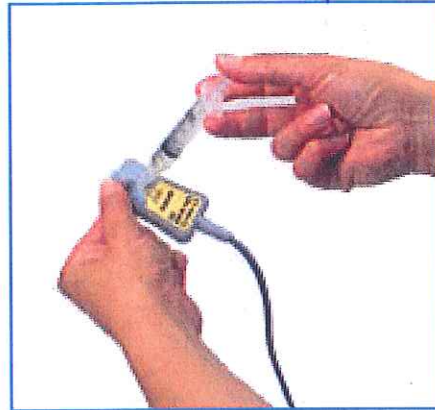





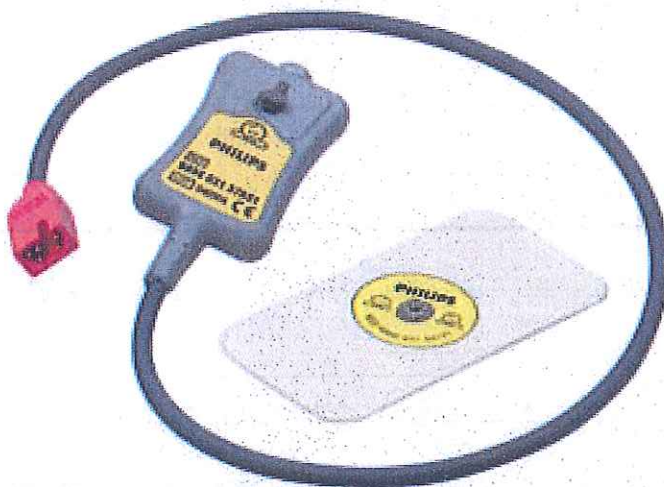


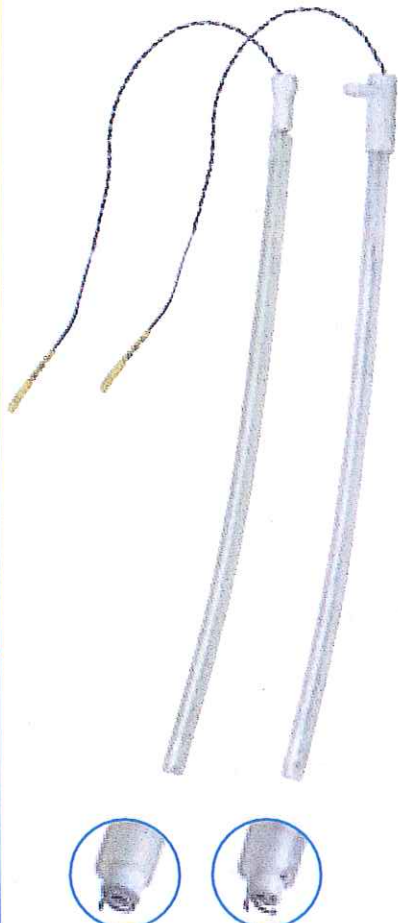





### Fast, easy cleaning

A convenient flushing port allows you to easily wash out the inner chamber.





**Component setup**

These monitors	connect to	with either of these spiral electrodes	
<p>Philips and legacy Hewlett-Packard/Agilent monitors</p>	<div style="display: flex; justify-content: space-around;"> <div style="text-align: center;">  <p>DECG transducer M1357A* 15240A*</p> </div> <div style="text-align: center;">  <p>DECG adapter M1347A</p> </div> </div> <hr/> <div style="display: flex; justify-content: space-around;"> <div style="text-align: center;"> <p>Patient module M1364A</p>  </div> <div style="text-align: center;"> <p>Avalon patient module M2738A</p>  </div> </div> <hr/> <div style="display: flex; justify-content: space-around;"> <div style="text-align: center;"> <p>Cordless ECG transducer M2727A</p>  </div> <div style="text-align: center;"> <p>Toco+ transducer M2735A</p>  </div> </div>	<p>DECG reusable legplate adapter cable 9898 031 37651</p> <p>Attachment electrode 9898 031 39771</p> 	<div style="display: flex; justify-content: space-around;"> <div style="text-align: center;"> <p>Fetal spiral electrode 9898 031 37631</p> </div> <div style="text-align: center;"> <p><b>OR</b></p> <p>Fetal double-spiral electrode** 9898 031 37641</p> </div> </div> 
<p>GE Corometrics 1xx series monitors and GE series 120 and 250 monitors (using a GE Corometric Y-adapter cable 1442AAO or socket adapter 1422BAO)</p>	<p>DECG reusable legplate adapter cable (round connector) 9898 031 37791</p> 	 	
<p>GE Corometrics</p> <ul style="list-style-type: none"> <li>• 120</li> <li>• 126</li> <li>• 128</li> <li>• 129</li> </ul>	<p>DECG reusable legplate adapter cable (rectangle connector) 9898 031 37801</p> 		
<p>Spacelabs</p> <ul style="list-style-type: none"> <li>• IM77***</li> </ul>	<p>DECG reusable legplate adapter cable 9898 031 37811</p> 		

\*Note: M1357A and 15240A are no longer available. The transducers have been replaced by the patient module M1364A which does not require an adapter.

\*\*Note: Available in Europe only

\*\*\*Other models of Spacelabs may require an additional adapter cable.

**Philips Healthcare is part of  
Royal Philips Electronics**

**How to reach us**

[www.philips.com/healthcare](http://www.philips.com/healthcare)

[healthcare@philips.com](mailto:healthcare@philips.com)

fax: +31 40 27 64 887

**Asia**

+852 2821 5888

**Europe, Middle East, Africa**

+49 7031 463 2254

**Latin America**

+55 11 2125 0744

**North America**

+1 425 487 7000

800 285 5585 (toll free, US only)

Philips Healthcare  
Global Information Center  
P.O. Box 1286  
5602 BG Eindhoven  
The Netherlands



© 2008 Koninklijke Philips Electronics N.V.  
All rights are reserved.

Philips Healthcare reserves the right to make changes in specifications and/or to discontinue any product at any time without notice or obligation and will not be liable for any consequences resulting from the use of this publication.

Printed in The Netherlands.  
4522 962 35411/864 \*JUN 2008